




Treatment Table – Re-Engaging Wheels

Please see below instruction to re-engage the wheel system on our treatment tables.

Instructions

Please ensure the wheels are facing lengthways down the table. You may need to roll the table a little so they are facing in the correct direction. Please see below example.

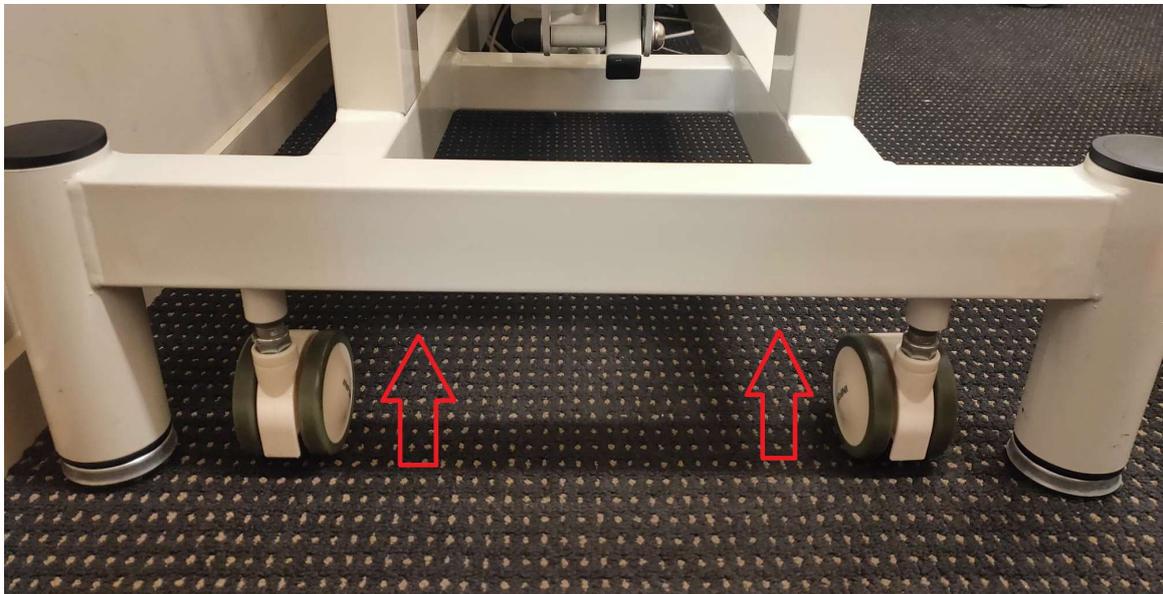

The next step is to pull the locking lever up and down quick approx. 5 times. Then push the lever back down to lock the wheels. This will re-engage the wheel system.



If your issues persist please contact Pacific Medical.

